



July 22nd, 2021

Mey GmbH & Co.KG
Uwe Scmid
Auf Steingen 6, D – 72459 Albstadt
Germany

Re: Celliant Testing Data Analysis – NO - 2708
Composition – 75% Cotton, 25% Celliant

Dear Uwe,

Fabric Sample: NO - 2708 was tested 3 times on TCPO2 and tested 2 times on ASH Analysis.

TCPO2 Results: 7.69 – 8.78% (minimum standard 7%) with all 3 passing.

ASH Results: 1.55% -1.55% (minimum standard .5%) with 2 passing.

The sample passed and is approved.

Detailed report is attached.


Thank you for your continued interest in our technology

Best regards,

Hologenix Department of Testing & Quality Assurance



THE EVOLUTION OF PERFORMANCE TECHNOLOGY

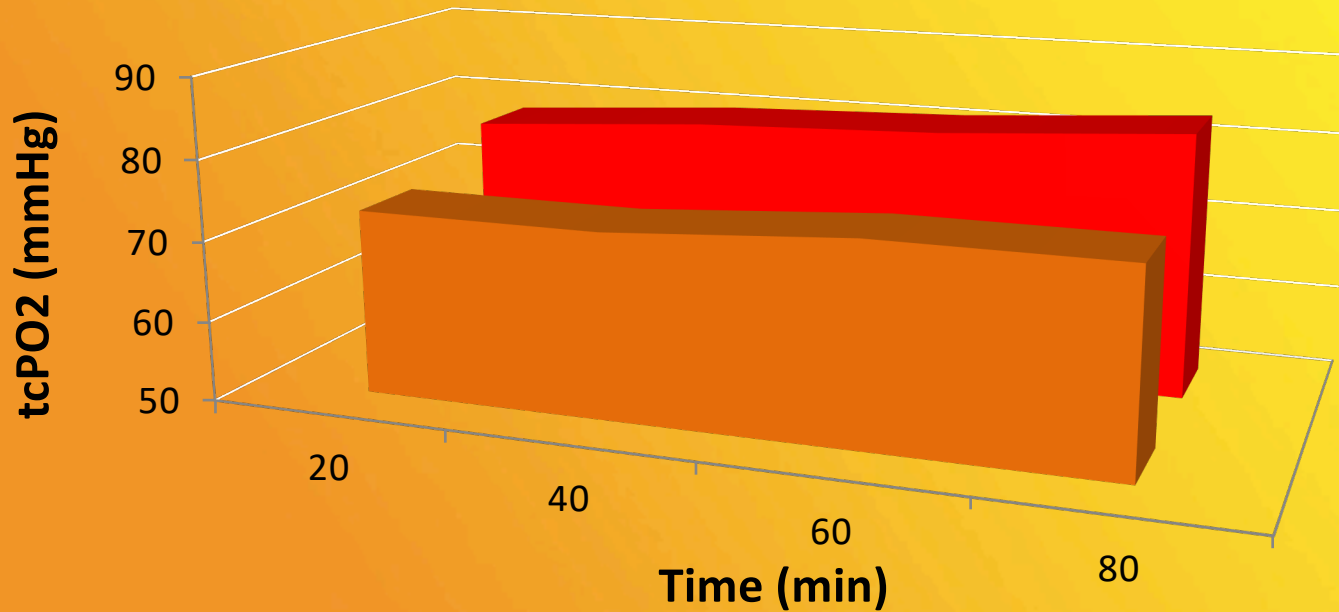

Average Increase
8.78%

	20	40	60	80
Placebo	73	73	75	75
Celliant	78	80	81	83

Test Sample

Mey GmBH

Style: NO-2708

Composition: 75% Cotton, 25% Celliant

Test Subject

M. Ramirez

Age: 29

Sex: Female

Weight: 140 lbs.

Room Temp: 74

Control Vitals

Skin Temp °C: 33.1
Blood Pressure: 129/81

Heart Rate: 60

Celliant Vitals


Skin Temp °C: 32.0
Blood Pressure: 134/85
Heart Rate: 65

Celliant Effect:

Time (Min)	Celliant
20	6.85%
40	9.59%
60	8.00%
80	10.67%

Hologenix, LLC
17383 Sunset Blvd Suite A420
Pacific Palisades, CA 90272

THE EVOLUTION OF PERFORMANCE TECHNOLOGY

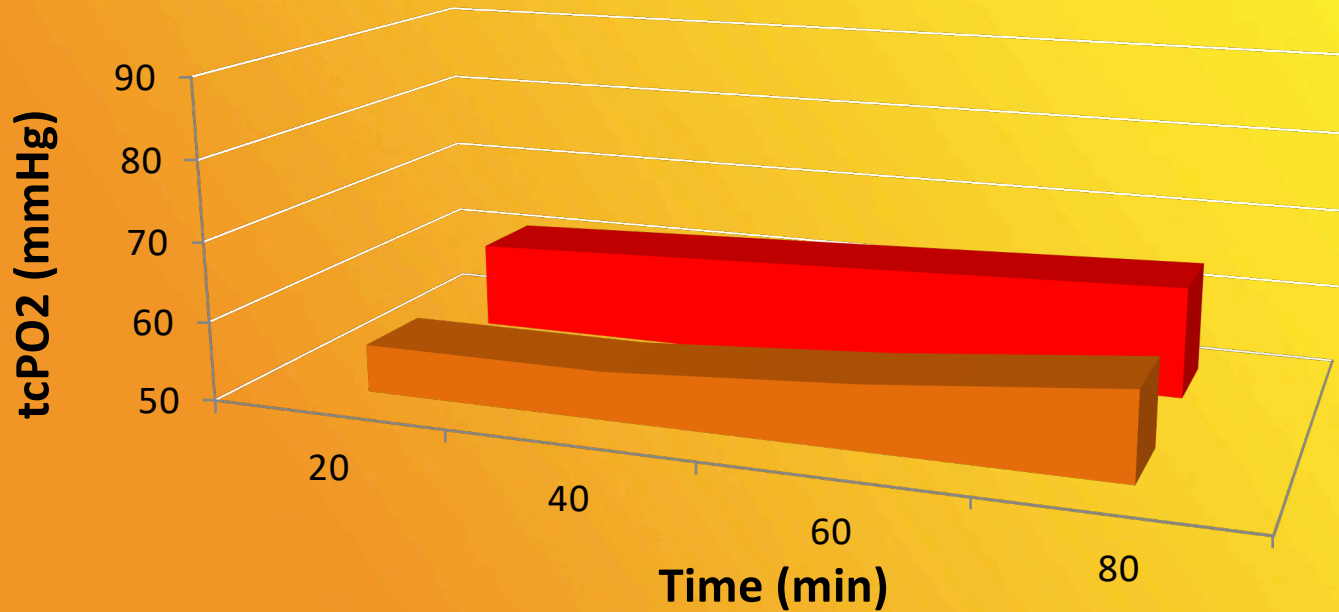

Average Increase
8.30%

	20	40	60	80
Placebo	56	56	58	61
Celliant	61	62	63	64

Test Sample

Mey GmBH

Style: NO-2708

Composition: 75% Cotton, 25% Celliant

Test Subject

T. Oselska

Age: 21

Sex: Female

Weight: 120 lbs.

Room Temp: 74

Control Vitals

Skin Temp °C: 33.1

Blood Pressure: 118/80

Heart Rate: 69

Celliant Vitals

Skin Temp °C: 33.5

Blood Pressure: 120/81


Heart Rate: 70

Celliant Effect:

Time (Min)	Celliant
15 - 25	8.93%
35 - 45	10.71%
55 - 65	8.62%
75 - 85	4.92%

Hologenix, LLC
17383 Sunset Blvd Suite A420
Pacific Palisades, CA 90272

THE EVOLUTION OF PERFORMANCE TECHNOLOGY

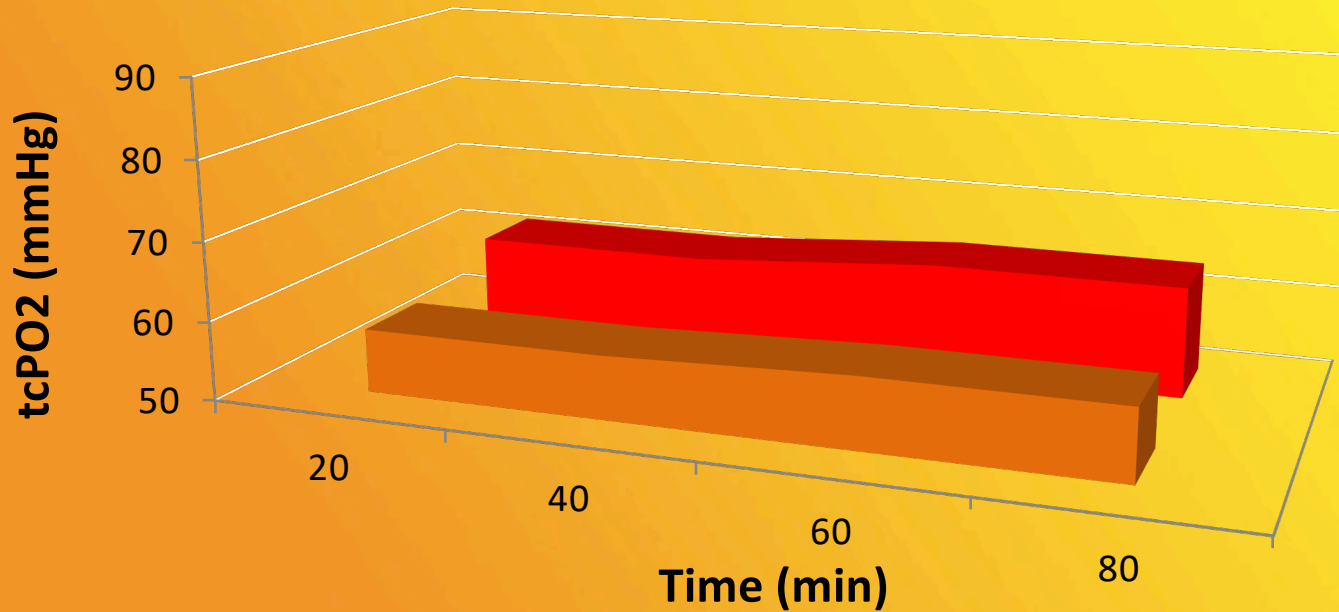

Average Increase
7.69%

	20	40	60	80
Placebo	58	58	59	59
Celliant	62	62	64	64

Test Sample

Mey GmbH

Style: NO-2708

Composition: 75% Cotton, 25% Celliant

Test Subject

F.Garlitos

Age: 67

Sex: Male

Weight: 220 lbs.

Room Temp: 74

Control Vitals

Skin Temp °C: 33.1

Blood Pressure: 121/83

Heart Rate: 66

Celliant Vitals

Skin Temp °C: 32.0

Blood Pressure: 121/81

Heart Rate: 70

Celliant Effect:

Time (Min)	Celliant
15 - 25	6.90%
35 - 45	6.90%
55 - 65	8.47%
75 - 85	8.47%

Hologenix, LLC
17383 Sunset Blvd Suite A420
Pacific Palisades, CA 90272

Laboratory Report

Report prepared for:

Lemekı Salusalu
Hologenix LLC
Suite A420
17383 Sunset Blvd
Pacific Palisade, CA 90272
Phone: 310-586-6828
Email: testing@celliant.com

Report prepared by:

Christy Love

Purchase Order:

CC,Casden,6/24/21

For further assistance, contact:

Christy Love
Report Coordinator
PO Box 51610
Knoxville, TN 37950 -1610
(865) 546-1335
christylove@galbraith.com

Sample: MEY GMBH NO-2708 BEIGE

Lab ID: 2021-N-7560

Received: 2021-06-24

Analysis	Method	Result	Basis	Sample Amount Used	Date (Time)
<i>115: Ash</i>					
	GLI Procedure G-45A	1.55 %	As Received	1385.72 mg	2021-06-29
	GLI Procedure G-45A	1.55 %	As Received	1537.79 mg	2021-06-29

Signatures:

Created By: Christy.Love

2021-06-30T19:50:38.177-04:00

Published By: Christy.Love

2021-06-30T19:50:45.773-04:00

- Physical signatures are on file.
- "Published By" signature indicates authorized release of data.



July 22nd, 2021

Mey GmbH & Co.KG
Uwe Scmid
Auf Steingen 6, D – 72459 Albstadt
Germany

Re: Celliant Testing Data Analysis – NO - 2709
Composition – 75% Cotton, 25% Celliant

Dear Uwe,

Fabric Sample: NO - 2709 was tested 3 times on TCPO2 and tested 2 times on ASH Analysis.

TCPO2 Results: 7.93 – 9.97% (minimum standard 7%) with all 3 passing.

ASH Results: 1.93% -1.97% (minimum standard .5%) with 2 passing.

The sample passed and is approved.

Detailed report is attached.


Thank you for your continued interest in our technology

Best regards,

Hologenix Department of Testing & Quality Assurance



THE EVOLUTION OF PERFORMANCE TECHNOLOGY

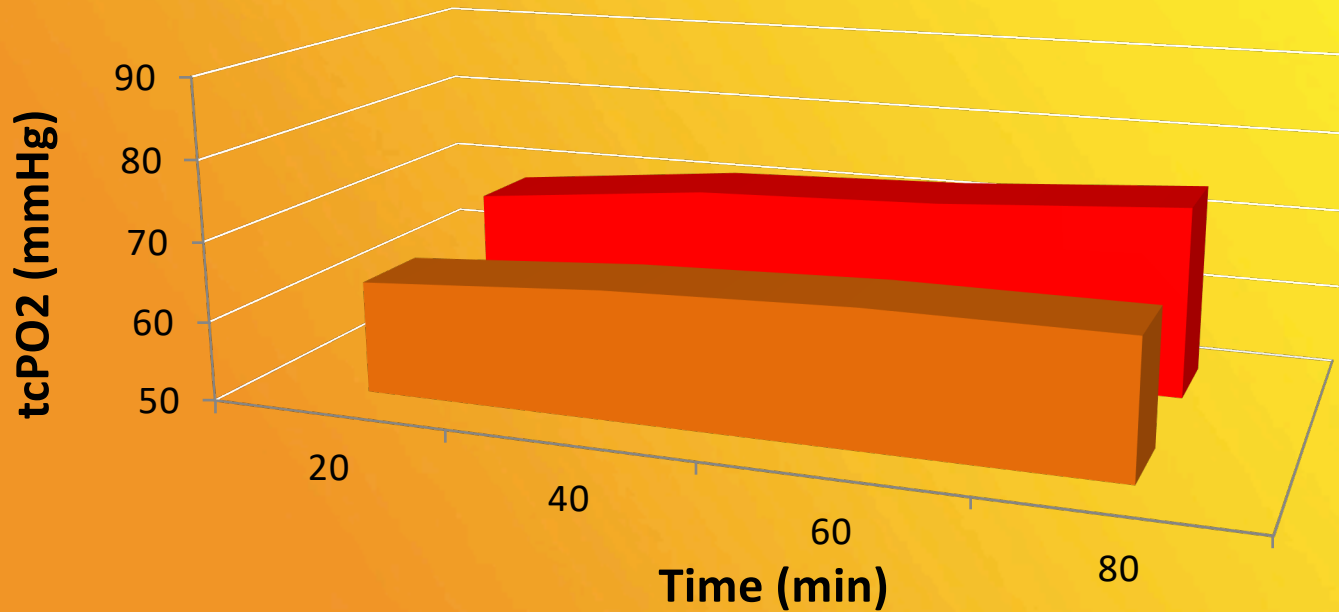

Average Increase
7.93%

	20	40	60	80
Placebo	64	66	67	67
Celliant	68	71	72	74

Test Sample

Mey GmBH

Style: NO-2709

Composition: 75% Cotton, 25% Celliant

Test Subject

M. Ramirez

Age: 29

Sex: Female

Weight: 140 lbs.

Room Temp: 74

Control Vitals

Skin Temp °C: 33.1
Blood Pressure: 129/81

Heart Rate: 60

Celliant Vitals


Skin Temp °C: 32.0
Blood Pressure: 134/85
Heart Rate: 65

Celliant Effect:

Time (Min)	Celliant
20	6.25%
40	7.58%
60	7.46%
80	10.45%

Hologenix, LLC
17383 Sunset Blvd Suite A420
Pacific Palisades, CA 90272

THE EVOLUTION OF PERFORMANCE TECHNOLOGY

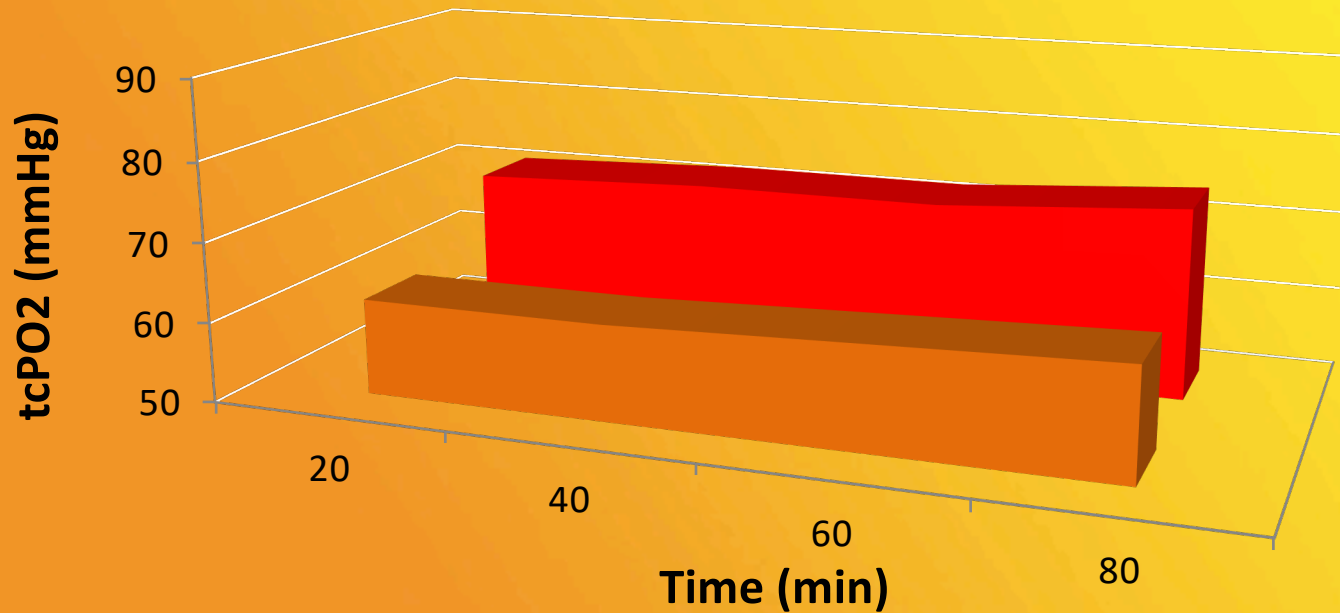

Average Increase
9.97%

	20	40	60	80
Placebo	62	62	63	64
Celliant	71	72	72	74

Test Sample

Mey GmBH

Style: NO-2709

Composition: 75% Cotton, 25% Celliant

Test Subject

T. Oselska

Age: 21

Sex: Female

Weight: 120 lbs.

Room Temp: 74

Control Vitals

Skin Temp °C: 33.1

Blood Pressure: 118/80

Heart Rate: 69

Celliant Vitals

Skin Temp °C: 33.5

Blood Pressure: 120/81


Heart Rate: 70

Celliant Effect:

Time (Min)	Celliant
15 - 25	9.68%
35 - 45	11.29%
55 - 65	9.52%
75 - 85	9.38%

Hologenix, LLC
17383 Sunset Blvd Suite A420
Pacific Palisades, CA 90272

THE EVOLUTION OF PERFORMANCE TECHNOLOGY

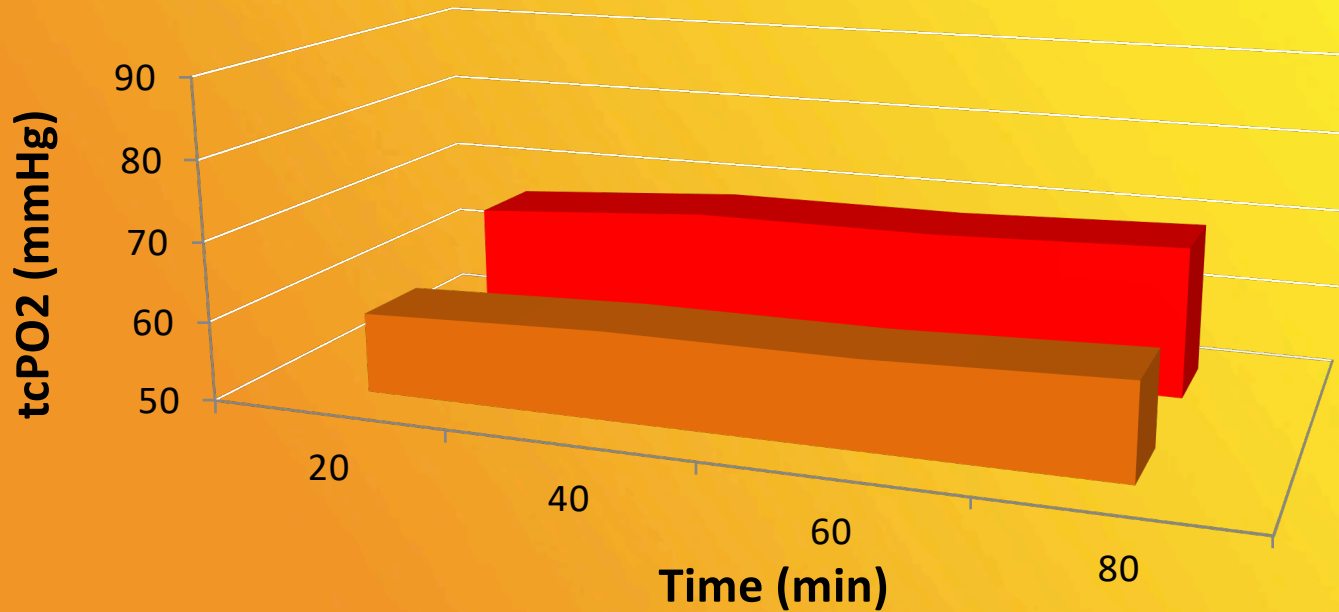

Average Increase
8.59%

	20	40	60	80
Placebo	60	61	61	62
Celliant	66	68	68	69

Test Sample

Mey GmbH

Style: NO-2709

Composition: 75% Cotton, 25% Celliant

Test Subject

F.Garlitos

Age: 67

Sex: Male

Weight: 220 lbs.

Room Temp: 74

Control Vitals

Skin Temp °C: 33.1

Blood Pressure: 121/83

Heart Rate: 66

Celliant Vitals

Skin Temp °C: 32.0

Blood Pressure: 121/81

Heart Rate: 70

Celliant Effect:

Time (Min)	Celliant
15 - 25	6.67%
35 - 45	8.20%
55 - 65	9.84%
75 - 85	9.68%

Hologenix, LLC
17383 Sunset Blvd Suite A420
Pacific Palisades, CA 90272

Laboratory Report

Report prepared for:

Lemeki Salusalu
Hologenix LLC
Suite A420
17383 Sunset Blvd
Pacific Palisade, CA 90272
Phone: 310-586-6828
Email: testing@celliant.com

Report prepared by:

Christy Love

Purchase Order:

CC,Casden,6/24/21

For further assistance, contact:

Christy Love
Report Coordinator
PO Box 51610
Knoxville, TN 37950 -1610
(865) 546-1335
christylove@galbraith.com

Sample: MEY GMBH NO-2709 BLACK

Lab ID: 2021-N-7559

Received: 2021-06-24

Analysis	Method	Result	Basis	Sample Amount Used	Date (Time)
<i>115: Ash</i>					
	GLI Procedure G-45A	1.93 %	As Received	1885.56 mg	2021-06-29
	GLI Procedure G-45A	1.97 %	As Received	1875.72 mg	2021-06-29

Signatures:

Created By: Christy.Love

2021-06-30T19:49:33.11-04:00

Published By: Christy.Love

2021-06-30T19:49:56.523-04:00

- ⓘ Physical signatures are on file.
- ⓘ "Published By" signature indicates authorized release of data.